

stryker

Together, let's **redefine** nailing.


Designed to **decrease** time and radiation

Guided distal locking designed to potentially reduce fluoroscopy and operative time.



Less inventory & storage space

Anatomically designed versatile nails require less inventory.

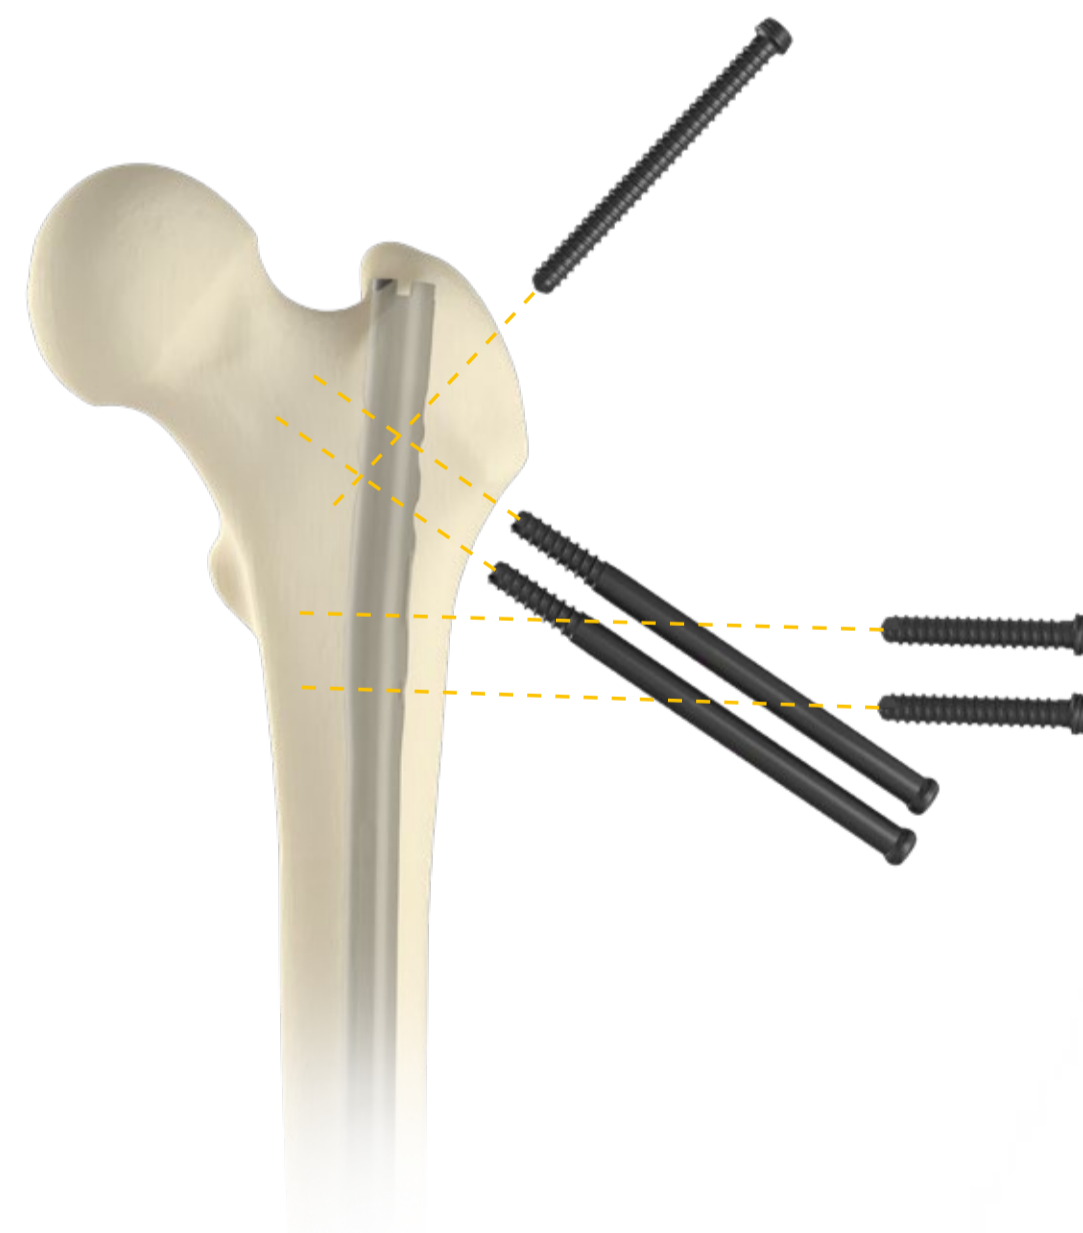

Quicker implant identification & presentation

Color-coded packaging designed for faster identification. Special sleeve allows aseptic implant handling.



More treatment options

Enhanced fragment fixation potentially reduces the risk of losing fracture reduction and the associated complications.



Shaped to **ease** implant placement

Length-dependant radius of curvature may provide better fit and reduce the risk of distal anterior penetration.

SOMA[®]

This document is intended solely for the use of healthcare professionals. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery. The information presented is intended to demonstrate a Stryker product. A surgeon must always refer to the package insert, product label and/or instructions for use, including the instructions for cleaning and sterilization (if applicable), before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area. Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Stryker, T2 Alpha. All other trademarks are trademarks of their respective owners or holders. Content ID: T2-PO-3, 08-2018 Copyright © 2018 Stryker

stryker.com